

Addendum to H₂Oil Analyzer System Product Manual, #70-82-25-100

Analyzer Enclosure Conduit Access

Some analyzer enclosures may have access holes in the pattern as shown in Figure 1 below. Install conduit and cabling in the manual according to Figure 1. If the hole pattern differs from Figure 1, refer to Page 37 in the product manual and follow the instructions to install conduit and cabling.

Conduit Installation

Wires connecting to the sensor assembly and the analyzer are to be routed through 1/2-inch and 3/4-inch rigid conduit. 3/4-inch NPT connections are provided on the sensor electronics and analyzer enclosures for conduit installation of the interconnecting cable. See Figure 1. See Table 14 for recommended cables, conduit and seal fittings suitable for analyzer installation. For hazardous location installation, see “*Hazardous Location Installation*”, Page 38.

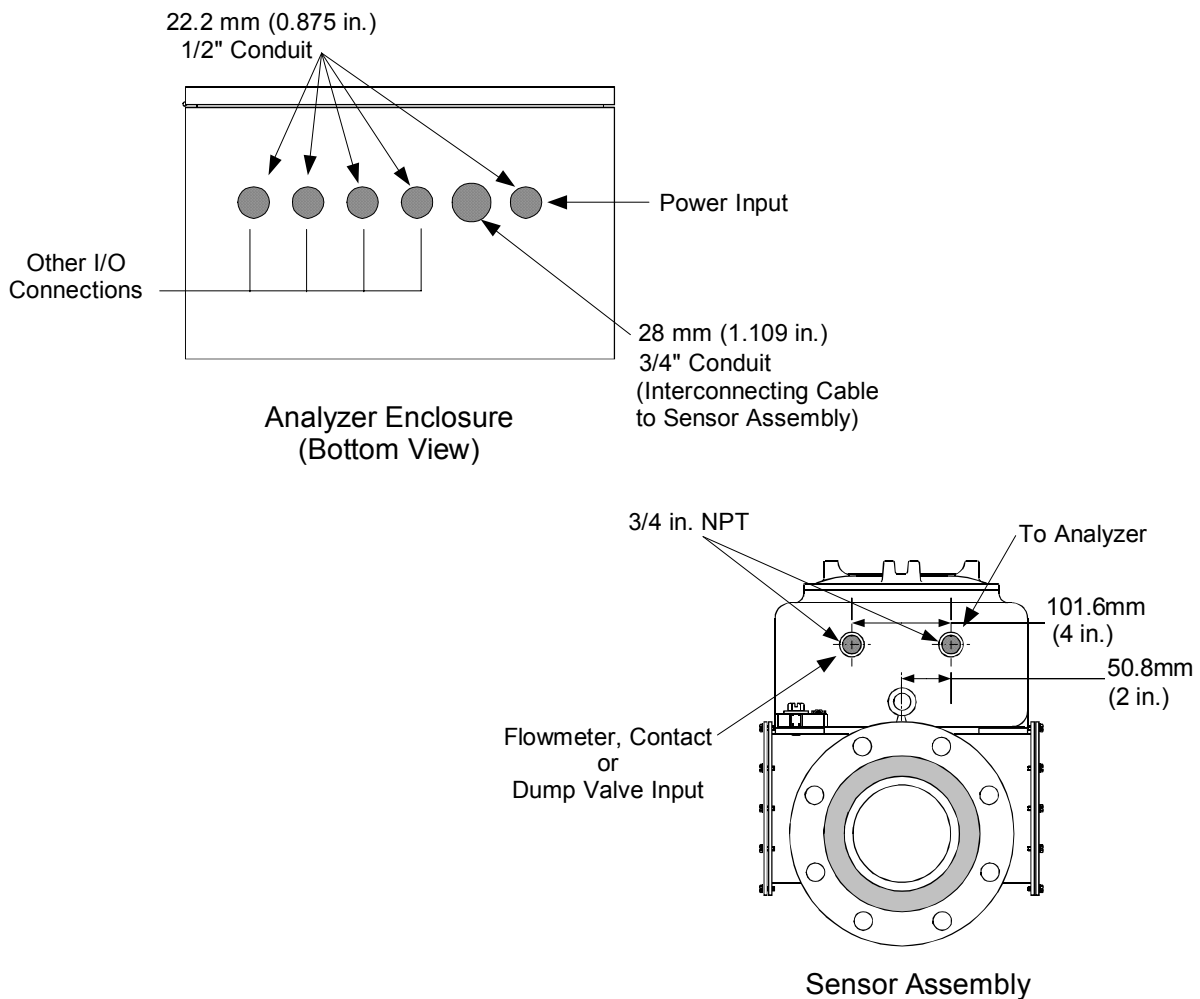


Figure 1 Conduit Connections